

**Project: IEEE P802.15 Working Group for Wireless Personal Area Networks (WPANs)**

**Submission Title:** [TG15.6 Regulation Summary]

**Date Submitted:** [May 15, 2008]

**Source:** [Huan-Bang Li]

Company [National Institute of Information and Communications Technology (NICT)]

**Contact:** Huan-Bang Li.

**Voice:**[+81 46 847 5104, E-Mail: lee@nict.go.jp]

**Abstract:** [A brief view on the TG15.6 related regulations]

**Purpose:** [To help forwarding the discussion in TG15.6]

**Notice:** This document has been prepared to assist the IEEE P802.15. It is offered as a basis for discussion and is not binding on the contributing individual(s) or organization(s). The material in this document is subject to change in form and content after further study. The contributor(s) reserve(s) the right to add, amend or withdraw material contained herein.

**Release:** The contributor acknowledges and accepts that this contribution becomes the property of IEEE and may be made publicly available by P802.15.

# TG 15.6 Regulation Summary

Huan-Bang Li

NICT, Japan

# Motivations

- **Present a brief view on the regulation subcommittee report**
- **Follow current undertaking on regulation**
- **Seeking for any complementary or new information,**

# Regulations Included In The Report

## ■ Countries and regions

- Australia, European Union, Japan, Korea, USA

## ■ Frequency bands

- Medical implant communication system (MICS)
- Wireless medical telemetry system (WMTS)
- Industrial, scientific, and medical band (ISM)
- Ultra-wideband (UWB)

# Frequency Band For MICS (402-405 MHz)

	Power	Channel	Remarks
Australia	< 25 $\mu$ W e.i.r.p	$\leq$ 300 kHz	Secondary use.
	< 100nW e.i.r.p	403.56 - 403.76 MHz	Medical implant telemetry systems
EU	< 25 $\mu$ W e.i.r.p	25 kHz/channel, one transmitter can use up to 300 kHz.	Secondary use.
Japan	< 25 $\mu$ W e.i.r.p	$\leq$ 300 kHz	Secondary use.
Korea	< 25 $\mu$ W e.i.r.p	$\leq$ 300 kHz	Secondary use.
	< 100nW e.i.r.p	403.5 -403.8 MHz	
USA	< 25 $\mu$ W e.i.r.p	$\leq$ 300 kHz	Secondary use.

# Frequency Band For MICS (401-402MHz and 405-406MHz)

- **In EU**, the 401-402 MHz and the 405-406 MHz frequency bands are allowed to be used for the emerging medical implant technologies, using Ultra Low Power – Active Medical Implants (ULP-AMI) and ULP-AMI-P (peripheral devices for ULP-AMI).
- The bandwidth can be from 25 kHz and up to 100 kHz with an e.i.r.p. of  $-25\mu\text{W}$ .

# Frequency Band For WMTS

	Frequency Bands	Bandwidths	Remarks
Australia	433.05–434.79 MHz	N/A	Low Interference Potential Devices
EU	N/A	N/A	N/A
Japan	420.05MHz – 449.6625 MHz	8.5 - 320 kHz	WMTS
Korea	N/A	N/A	N/A
USA	608 – 614 MHz 1395 – 1400 MHz 1427 -1729.5 MHz	1.5 – 6 MHz No specification No specification	WMTS

# UWB Low Bands


	PSD	Frequency Bands	Remarks
Australia	N/A	N/A	N/A
EU	-41.3 dBm/MHz	3.4 - 4.8 GHz	LDC or DAA are applied
		4.2 - 4.8 GHz	By Dec. 31, 2010
Japan	-41.3 dBm/MHz	3.4 – 4.8 GHz	DAA is applied
		4.2 – 4.8 GHz	By Dec. 31, 2008
Korea	-41.3 dBm/MHz	3.1 - 4.8 GHz	LDC or DAA are applied
		4.2 - 4.8 GHz	By Dec. 31, 2010
USA	-41.3 dBm/MHz	3.1 -10.6 GHz	
Common	-41.3 dBm/MHz	4.2 -4.8 GHz	Time limitation



# UWB High Bands

	Frequency Bands	PSD	Remarks
Australia	N/A	N/A	N/A
EU	6 - 8.5 GHz	-41.3 dBm/MHz	
Japan	7.25 – 10.25 GHz	-41.3 dBm/MHz	
Korea	7.2 -10.2 GHz	-41.3 dBm/MHz	
USA	3.1 -10.6 GHz	-41.3 dBm/MHz	
Common	7.25 -8.5 GHz	-41.3 dBm/MHz	

# UWB Band Highlight

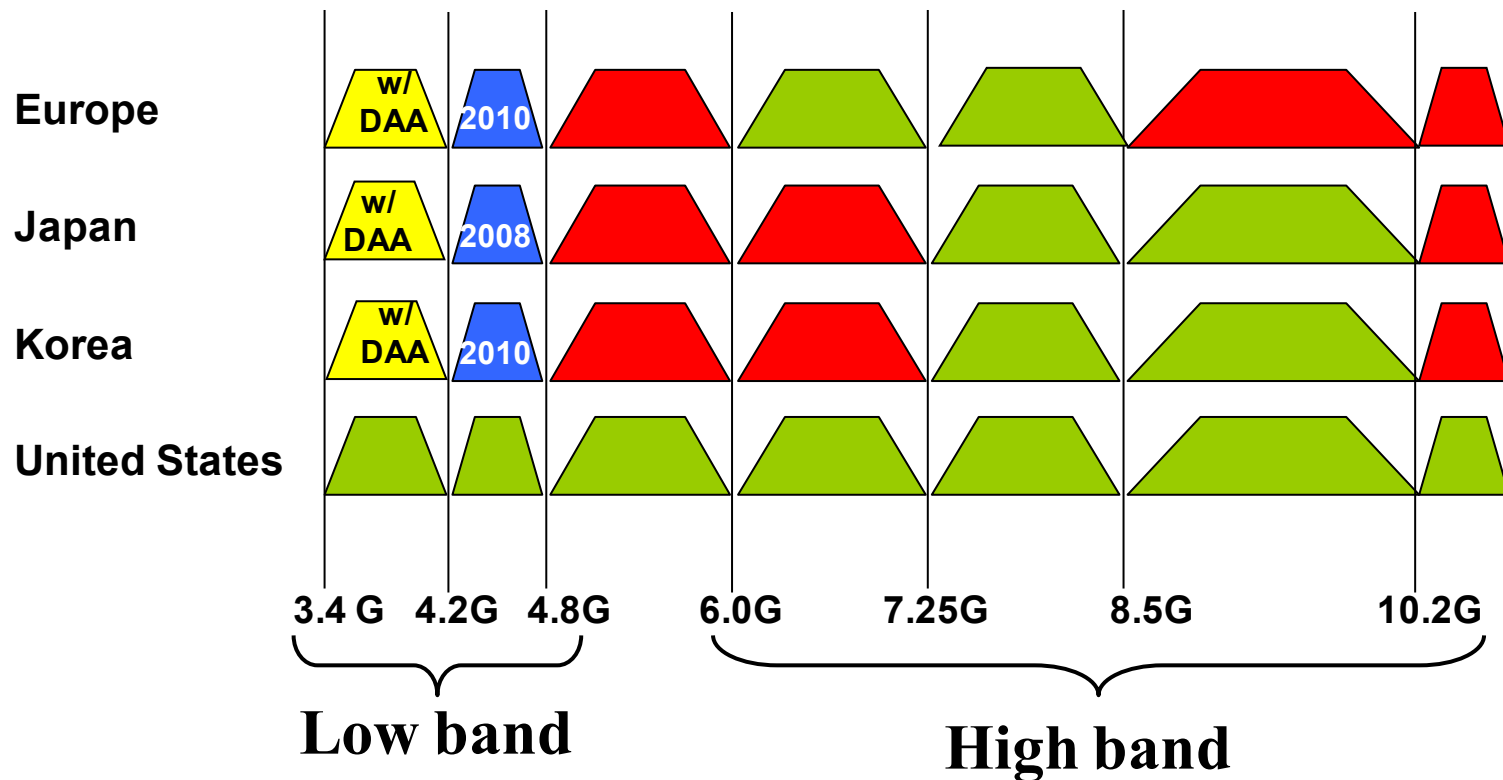


⊛ Currently, the data rate must be larger than 50 Mbps for UWB technology as required by Japanese regulation.

# ISM Bands

The ISM bands are allocations for unlicensed operation. The interested ISM bands include

- 433.05–434.79 MHz (centre frequency 433.92 MHz)
- 2.400–2.500 GHz (centre frequency 2.450 GHz)
- 5.725–5.875 GHz (centre frequency 5.800 GHz)

# Frequency Band Highlight

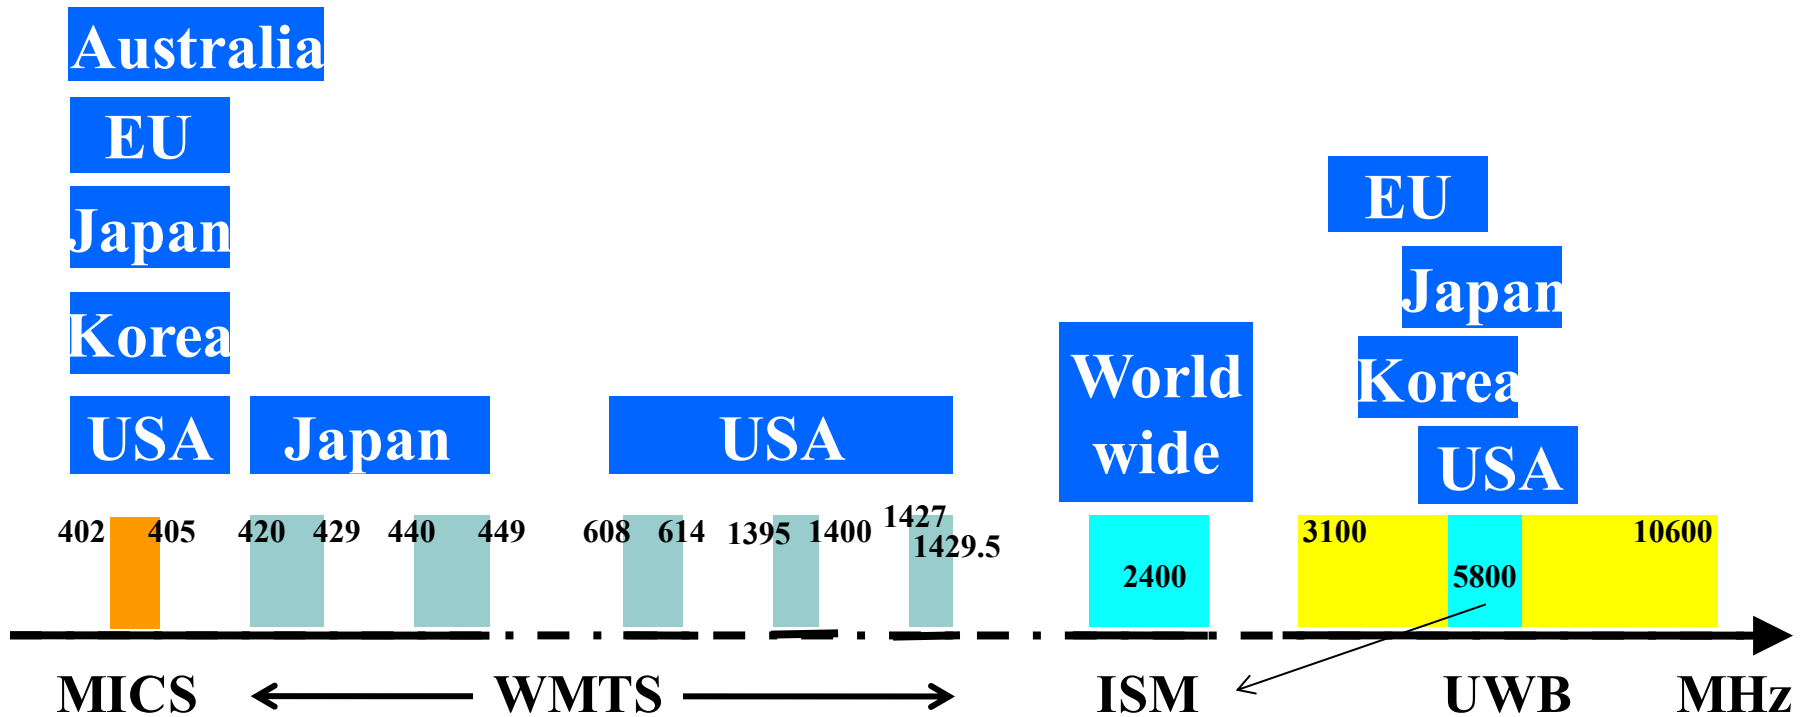

# FCC NPRM and NOI

- July 18, 2006, FCC released Notice of proposed rulemaking (**NPRM**) and notice of inquiry (**NOI**) document [**FCC-06-103**]

✓ 402-405 MHZ  
✓ MICS use only

Current

✓ 401-406 MHZ  
✓ MedRadio = Medical  
radio communication

New

# FCC Public Notice (April 2008)

It follows the GE Healthcare's ex parte

- Proposed frequency band for MBAN (2360 -2400 MHz)
  - 2370 – 2390 MHz for **an inner set**
  - 2360 – 2370 MHz } for **an out set**
  - 2390 – 2400 MHz }

**Proposed emission power is up to 0 dBm for a maximum 1MHz bandwidth.**

**Any related information is  
appreciated**

**and**

**Thank you for your attention !**